


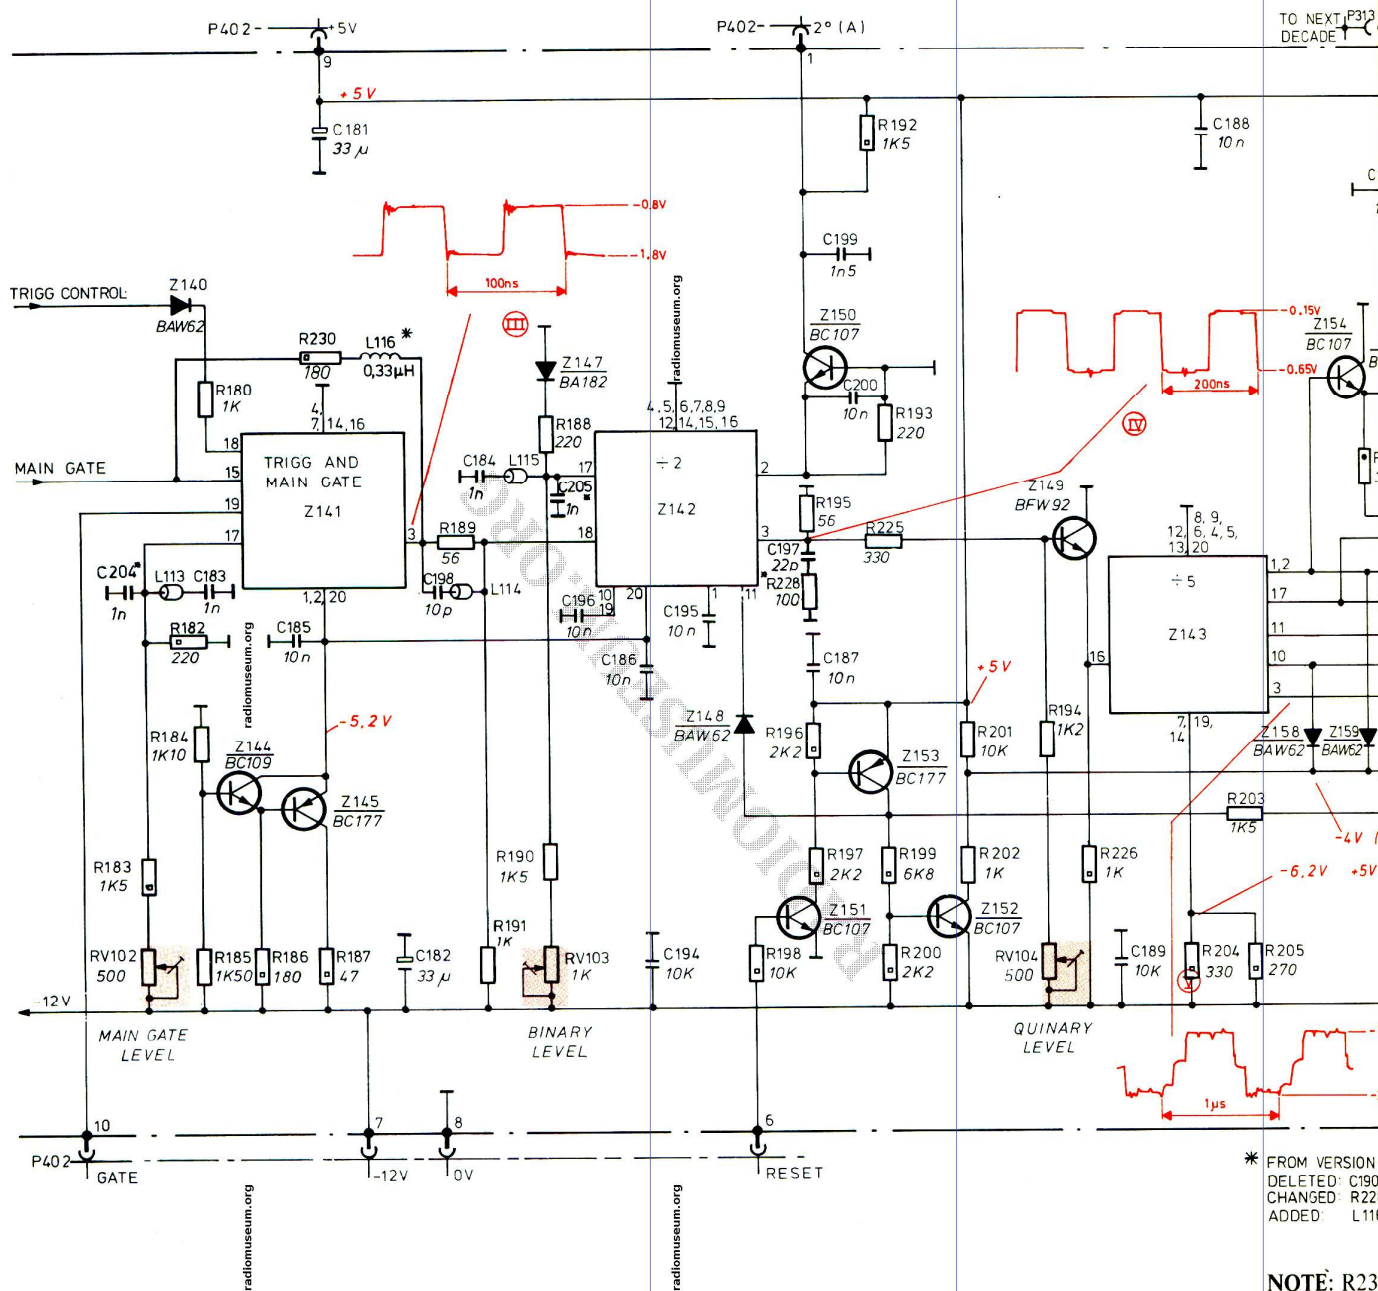

* FROM VERSION -
DELETED: C190
CHANGED: R228
ADDED: L116

NOTE: R230
R225

TEST CONDITIONS

If not otherwise stated, the following test conditions apply:
Measuring mode: FREQUENCY
Gate time: 10 ms
INT/EXT time base switch S413: INT
10 MHz signal is taken from rear panel connector
10 MHz OUT, P26, and applied to INPUT A, P11.
D.C. voltages are measured without input signal.

TEST INSTRUMENTS USED

Waveform displays: PHILIPS sampling oscilloscope
PM 3400 with passive probe 1:10,
PM 9342.
D.C. voltages : Multimeter 40,000 Ω /V, PHILIPS
PM 2411

VOLTAGES AND WAVEFORMS ARE TYPICAL.